



Measurement of Available Footpath

- a) There must be a minimum width of unobstructed footway of 2.0 metres between the edge of the trading area and 200mm from the edge of the footway. The 200mm distance is to allow for the fact that pedestrians cannot be expected to walk on the edge of the footpath.

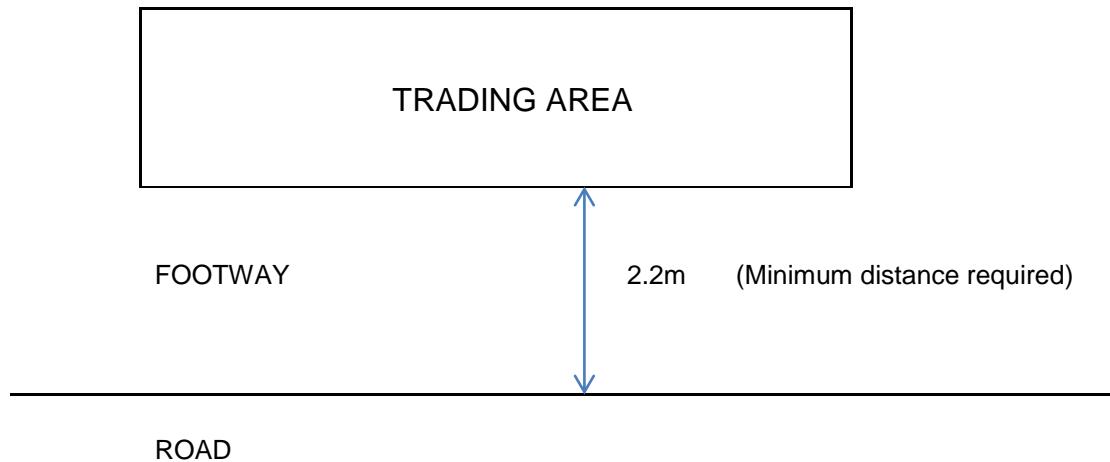

- b) Please note that the measurement is taken from the edge of the trading area and not the receptacle that may be used for trading. This is to allow for people browsing or queuing at the trader and not interfering with passing pedestrians.
- c) Where pedestrian flow rates are greater than 1200 persons per hour, particularly near a tourist attraction, this distance may be increased taking into consideration the likelihood of pedestrians stopping to observe shop fronts/the attraction etc. There is no exact formula for determining the minimum width of footpath and each case will be determined on its merits. The overriding factor will be the comfort of pedestrians and their ability to pass along the footpath safely.

- d) Where the footpath contains other street furniture such as lamp posts, bollards, parking meters, telephone booths, benches etc., the minimum unobstructed width will be measured between the edge of the trading area and 200mm from the item(s) in question plus the additional distance between the item(s) and 200mm from the edge of the footpath if each distance is not less than 1.2 metres.

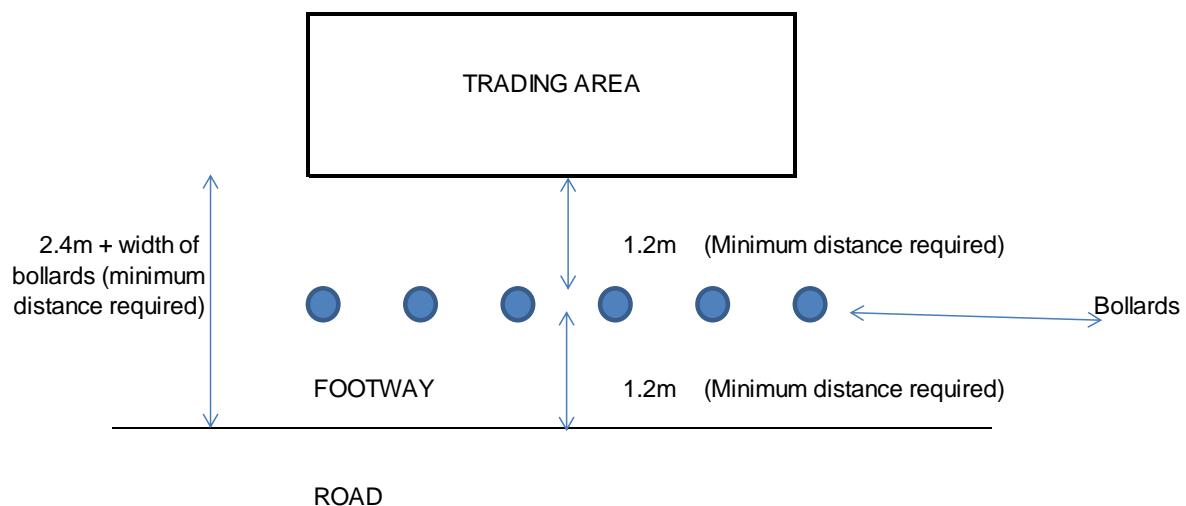

- e) The positioning of the trading area should never discourage pedestrians from using the footway. The available pedestrian route must be straight, obvious and unobstructed and not pass through the trading area. An exception may be made where a street market occupies the whole of the Trading Area and the pedestrian route passes through the centre of that market.